



KB03005
BCA Protein
Quantification
Assay Kit

200/1000 tests (96 well plate)
28/140 tests (test tube)

Table of contents

1.	General information	1
2.	Technical specifications	2
3.	Materials and storage	3
4.	Introduction	4
5.	Assay principle	4
6.	Assay preparation	5
7.	Sample preparation	7
8.	Assay protocol	8
9.	Data analysis	10
10.	Troubleshooting	12
11.	Additional information	14
12.	Related products	14
13.	Warranties and limitation of liability	15

1. General information

PRECAUTIONS

Please read this manual carefully before beginning the assay.

This product is designed for **research use only**. It is not approved for human or animal use or clinical diagnosis. All chemicals should be handled with care and in accordance with laboratory safety practices. It is recommended to use basic Personal Protective Equipment.

Do not use after the expiration date stated on the packaging.

Do not mix or substitute reagents or materials from other kit batches or vendors.

For the **material safety data sheet** (MSDS) please contact us at info@bioquochem.com

TECHNICAL RECOMMENDATIONS

Store reagents as indicated in **Materials and storage** section.

Be sure to keep the bottle capped when not in use.

Let the components reach room temperature (RT) before use.

Immediately before use, gently invert and rotate reagent bottles several times to mix the contents thoroughly.

Avoid foaming or bubbles when mixing or reconstituting components.

Avoid cross contamination of samples or reagents by changing pipette tips between sample, standard and reagent additions.

Be sure to use the optimal microplate for the assay. Flat bottom transparent microplates for UV/VIS applications, and black microplates for fluorescence measurements.

2. Technical specifications

Available sizes

Test tube format: 28/140 tests

Microplate format: 200/1000 tests

Required sample volume

Test tube format: 75 μ L/test

Microplate format: 10 μ L/test

Compatible samples

Biological fluids, food, and beverages

Type of detection

Colorimetric (562 nm)

3. Materials and storage

MATERIALS SUPPLIED

Item	No. Tests	Units	Storage
Reagent A	200	1	RT
	1000	5	
Reagent B	200	1	RT
	1000	1	
Protein Standard	200	1	4 °C
	1000	2	
Transparent 96-Well Microplate	200	2	RT
	1000	4	
	1000	4	

MATERIALS NEEDED BUT NOT SUPPLIED

- Double distilled water (ddH₂O) as Milli-Q Ultrapure Water.
- Labware materials (micropipettes, tubes, stirring/mixing equipment).
- Colorimetric microplate reader – equipped with filter for OD 562 nm.

STORAGE CONDITIONS

On receipt, store kit components as indicated above. Under these conditions, the reagents are stable in the original packaging until the expiration date indicated on the outside of the box. After reconstitution, protein standard solution should be stored at -20 °C. Prepare a fresh set of standards for every use.

4. Introduction

The bicinchoninic acid (BCA) assay is a protein quantification technique that was first described by Paul K. Smith in 1985.

Proteins are biopolymeric structures composed of amino acids that play many critical roles in the body. Protein is also a vital part of the human diet. Protein quantification assays are therefore fundamental to biological research, clinical diagnosis or food industry.


The BCA assay has many advantages over the alternatives (e.g. Lowry, Bradford) including compatibility with a wide variety of detergents, stability of the chromophore and protein-to-protein uniformity.

BQC BCA Protein Quantification Assay Kit is a simple test for the quantification of proteins in a wide variety of samples.

5. Assay principle

BQC BCA Protein Quantification Assay Kit is based on the bicinchoninic acid (BCA) assay.

This method relies on two chemical reactions. The first is the Biuret reaction, in which Cu^{2+} is reduced to Cu^+ by proteins in an alkaline solution. The second reaction is the chelation of reduced copper ions by bicinchoninic acid to produce a purple complex with strong absorbance at 562 nm. The protein concentration in a sample is determined from a calibration curve using bovine serum albumin (BSA) as standard.

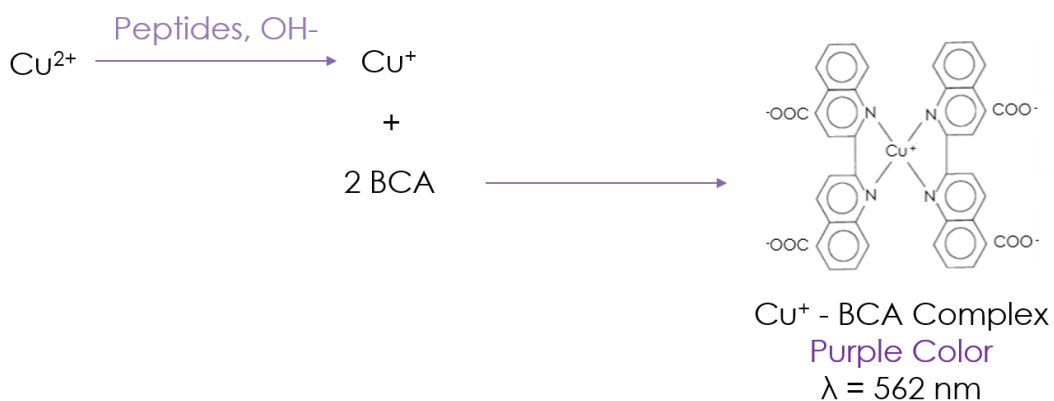

Principle of the BCA Assay Kit

6. Assay preparation

REAGENT PREPARATION

All assay reagents not listed below are ready to use as supplied. Allow the reagents to reach room temperature before use.

BCA Working Solution: Mix Reagent A with Reagent B in a 50:1 ratio (e.g. for preparing 20 mL of BCA WS mix 19.6 mL of Reagent A and 0.4 mL of Reagent B).

- ⓘ **CAUTION:** BCA Working Solution (BCA WS) must be prepared immediately before use. Before preparing **BCA WS** consider the number of tests to be performed and therefore the volume of solution required. Use the following formula to determine the total volume of BCA WS required:

Volume BCA WS=(Standards+Samples)x(Number Replicates)x(Volume BCA WS/test*)

*1425 µL test tube format/ 200 µL microplate format

Protein Standard Solution (Bovine Serum Albumin, BSA): Add 3 mL of ddH₂O to the Standard vial. Mix carefully to avoid foaming.

- ⓘ **NOTE:** Aliquot and store at -20 °C the Standard Solution for long term use.

STANDARD CALIBRATION

Test tube BCA Protein Quantification Kit

Prepare BSA standards for the calibration curve from the Standard solution according to the following Table. Prepare the standards immediately prior to each assay. Mix carefully to avoid foaming.

Standard	Standard solution (µL)	*Diluent (µL)	Protein (µg/mL)
Std 1 (Reagent Blank)	0	300	0
Std 2	6	294	200
Std 3	12	288	400
Std 4	24	276	800
Std 5	36	264	1200
Std 6	48	252	1600

*Use as diluent the buffer used in the samples

Microplate BCA Protein Quantification Kit

Prepare BSA standards for the calibration curve from the Standard solution according to the following Table. Prepare the standards immediately prior to each assay. Mix carefully to avoid foaming

Standard	Standard solution (µL)	*Diluent (µL)	Protein (µg/mL)
Std 1 (Reagent Blank)	0	200	0
Std 2	4	196	200
Std 3	8	192	400
Std 4	16	184	800
Std 5	24	176	1200
Std 6	32	168	1600

*Use as diluent the buffer used in the samples

PLATE SET UP

BQC recommends running the standards and samples at least in duplicate (triplicate recommended). There is no specific pattern for using the wells on the plate. A proposed layout of standards (Std) and samples (S) to be measured in duplicate is shown below.

NOTE: If sample blanks are included in the assay, it is necessary to reserve some wells of the plate for these blanks

	1	2	3	4	5	6	7	8	9	10	11	12
A	Std 1	Std 1	S3	S3	S11	S11	S19	S19	S27	S27	S35	S35
B	Std 2	Std 2	S4	S4	S12	S12	S20	S20	S28	S28	S36	S36
C	Std 3	Std 3	S5	S5	S13	S13	S21	S21	S29	S29	S37	S37
D	Std 4	Std 4	S6	S6	S14	S14	S22	S22	S30	S30	S38	S38
E	Std 5	Std 5	S7	S7	S15	S15	S23	S23	S31	S31	S39	S39
F	Std 6	Std 6	S8	S8	S16	S16	S24	S24	S32	S32	S40	S40
G	S1	S1	S9	S9	S17	S17	S25	S25	S33	S33	S41	S41
H	S2	S2	S10	S10	S18	S18	S26	S26	S34	S34	S42	S42

Example of plate layout for the BCA Protein Quantification Assay Kit

7. Sample preparation

The following sample preparation protocols are intended as a guide only. The optimal conditions for sample preparation must be determined by the end user. It is recommended to use fresh samples. If it is not possible, aliquot and store samples appropriately with minimal freeze/thawing.

BCA Protein Quantification Assay Kit can be used to determine proteins in a wide variety of samples like biological fluids, food, and beverages.

Reagents and materials required for sample preparation are not supplied with the kit. Before doing sample preparation, consider the volume of sample required per test; see **Technical specifications** section.


Make sure that interfering substances present in the sample do not give a significant background. Run proper blanks as necessary (e.g. sample blank should be always evaluated when working with highly colored samples). It is recommended to assay different sample dilutions to ensure the values fall within the standard curve.

8. Assay protocol

Prepare and mix all reagents thoroughly before use. Each standard, sample or blank should be assayed at least in duplicate.

Test tube BCA Protein Quantification Kit (1.5 mL)

1



Pipette **75 μ L** of **standard** or **sample** into 1.5 mL microcentrifuge tubes (not included)

2



Add **1425 μ L** of **BCA Working Solution** to each tube and mix well

3



Incubate the tubes for **15 minutes** at **60 °C**

4



Let the tubes **reach RT**


5



Read the **absorbance** at **562 nm**

Microplate BCA Protein Quantification Kit

1



Set up the plate design

2



Add **10 μ L** of **standard** or **sample** in each well

3



Add **200 μ L** of **BCA Working Solution** in each well and mix by pipetting

4



Incubate the microplate for **15 minutes** at **60 °C**

5



Let the microplate reach **RT**

6




Read the **absorbance** of all wells at **562 nm** at **RT**

9. Data analysis

ANALYSIS OF THE STANDARDS

- Calculate the average absorbance of the standards.
- Subtract the average absorbance of the reagent blank (Std 1) from the average absorbance of the standards to obtain the blank-corrected absorbance of the standards.
- Create a standard curve by plotting the blank-corrected absorbance of the standards as a function of the standard concentration (see **STANDARD CALIBRATION** section). A typical standard curve ($y = \text{slope} \cdot x \pm \text{intercept}$) for the microplate assay procedure is shown below.

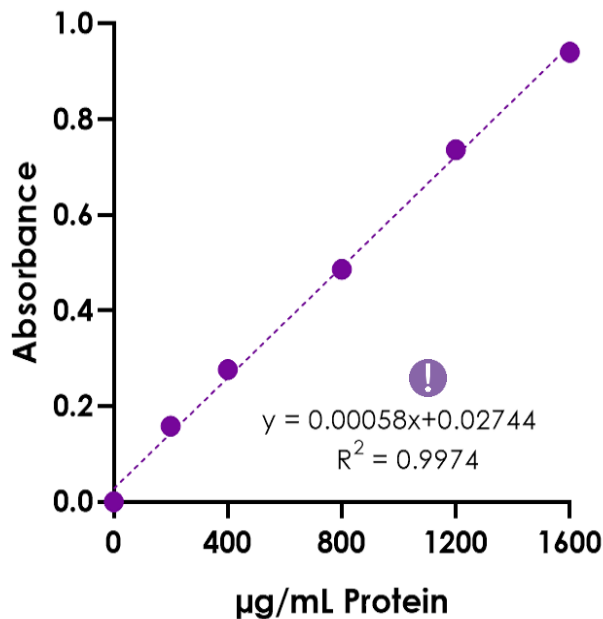

Protein standard curve with BCA Quantification Assay Kit

- ⚠ This standard curve is an example of the data typically obtained with this kit. **DO NOT USE** this standard curve to calculate the protein concentration of your samples. A new standard curve must be performed by the end user.

ANALYSIS OF THE SAMPLES

- Calculate the average absorbance of the samples.
- Subtract the average absorbance of the reagent blank (Std 1) from the average absorbance of each sample to obtain the blank-corrected absorbance of the samples.
- Calculate the protein concentration of the samples using the following equation. Slope and intercept values are obtained from the standard curve.

$$\text{Protein } (\mu\text{g/mL}) = \left(\frac{A_s - \text{intercept}}{\text{slope}} \right)$$

When working with diluted samples the concentration values obtained must be multiplied by the dilution factor to obtain the protein concentration of the undiluted sample.

10. Troubleshooting

This troubleshooting table provides potential sources and solutions for common problems observed with BQC Assay Kits. **The problems listed below could occur when using any BQC Assay Kit.** They are not specific for this assay kit.

Problem	Possible Cause	Recommended Solution
Wells have color but there is no reading	Plate read at incorrect wavelength	Check the wavelength used in the assay
	Incorrect microplate	Use the correct microplate for your application UV/Vis: transparent Fluorescence: black wells/transparent bottom
Standard readings do not follow a linear pattern	Pipetting errors in preparation of standards	Avoid pipetting small volumes (<5 μ L) Be careful not to splash from well to well
	Air bubbles formed in well(s)	Use reverse pipetting technique
	Standard stock is at incorrect concentration	Always refer to dilutions described in Assay preparation
	Improperly thawed reagents	Thaw all components completely and mix well before use
	Use of improperly stored reagents	Store the components appropriately Use fresh components from the standard curve
	Incorrect incubation times or temperatures	Refer to Assay protocol
Dispersion of standard and sample readings	Pipetting errors	Avoid pipetting small volumes (<5 μ L) Be careful not to splash from well to well
	Air bubbles formed in well(s)	Use reverse pipetting technique

Problem	Possible Cause	Recommended Solution
Sample erratic values	Samples contain interfering substances	Dilute sample further (if possible)
	Inappropriately stored samples or samples used after multiple freeze-thaw cycles	Use fresh samples or store appropriately until use
	Samples not deproteinized	Use an appropriate deproteinization protocol
	Cells/Tissue samples not homogenized completely	Repeat the sample homogenization
	Inappropriate sample dilution buffer	Refer to Assay preparation
Sample reading fall outside the detection range	Samples are too diluted/concentrated No analyte/activity is observed in the sample	Re-assay using different sample dilutions

STILL HAVING PROBLEMS?

Contact BQC if you have any further questions, our team will be pleased to help you:



Phone + 34 985 26 92 92



E-mail info@bioquochem.com



Business hours
Monday-Thursday: 8.30 to 17.00 (CEST)
Friday: 8.00 to 15.00 (CEST)

11. Additional information

BCA Protein Quantification Assay Kit is a fast, simple and precise assay (RSD <10 %) for determining proteins in a wide variety of samples.

Some reagents including detergents at high concentration, chelating agents, strong acids, or bases, and reducing agents, have been reported to interfere with this assay and must be avoided.

If unexpected results are obtained running your samples, please contact us at info@bioquochem.com

12. Related products

More products available on bioquochem.com

Reference	Product
KF03003	Bradford Protein Quantification Assay Kit
KF01001	DMPD Antioxidant Capacity Assay Kit
KB03002	Lipid Peroxidation Assay Kit

13. Warranties and limitation of liability

BQC shall not in any event be liable for incidental, consequential or special damages of any kind resulting from any use or failure of the products, even if BQC has been advised of the possibility of such damage including, without limitation, liability for loss of use, loss of work in progress, downtime, loss of revenue or profits, failure to realize savings, loss of products of buyer or other use or any liability of buyer to a third party on account of such loss, or for any labor or any other expense, damage or loss occasioned by such product including personal injury or property damage is caused by BQC's gross negligence. Any and all liability of BQC hereunder shall be limited to the amounts paid by the buyer for the product.

Buyer's exclusive remedy and BQC's sole liability hereunder shall be limited to a refund of the purchase price, or the replacement of all material that does not meet our specifications.

Said refund or replacement is conditioned on buyer giving written notice to BQC within 30 days of shipment.

Expiration date: 1 year from the date of fabrication. Expiration date is indicated on the outside of the box.

For further details, please refer to our website bioquochem.com



Edificio CEEI | Parque Tecnológico de Asturias,

33428 Llanera, Asturias

Info@bioquochem.com



www.bioquochem.com