

Technical Information

Protein A-R28 is an alkali-tolerant IgG-binding protein derived from protein A, which is developed with ProteNova's patent technology. Protein A-R28 strongly binds to various species and subclasses of IgG, compared with Protein A and G. The coupling to resin (Ab-Capcher) provides an alkali-washable unique affinity medium with high binding capacity for immunoglobulin, which is useful for purification of human, rabbit, mouse and rat IgGs. Ab-Capcher is also useful for immuno-precipitation experiments.

Table 1. Binding properties of Ab-Capcher (Ab-Rapid PuRe)

Species	Sub class	Ab-Cap	Protein A	Protein G
Mouse	IgG1	++++	+	++
	IgG2a	+++++	++++	+
Rat	IgG1	++++	-	+
	IgG2a	+++	-	+
Goat	IgGs	++++	-	+
Chicken	IgY	-	-	-
Human	IgG	+++++	++++	++
Rabbit	IgG	+++++	++++	++

Ab-Rapid PuRe™

Users Manual

Order Information

Product name	Contents	Code No.
• Ab-Rapid PuRe 2	Column x 2, 2.5 mL syringe x 1	P-012-2
• Ab-Rapid PuRe 10	Column x 10	P-012-10
• Buffer Kit	Bind. Buf. 200 mL, Elut. Buf. 30 mL, Neutr. Buf. 1mL	P-011

Related products

Product name	Contents	Code No.
• Ab-Capcher	2 mL	P-002-2
	10 mL	P-002-10
• Ab-Rapid SPiN 10	0.1mL spin column x 10	P-013-10
• Ab-Rapid SPiN 50	5 mL gel x 1, empty spin column x 50	P-013-50



COSMO BIO CO., LTD.


Inspiration for Life Science

TOYO EKIMAE BLDG. 2-20, TOYO 2CHOME
KOTO-KU, TOKYO 135-0016, JAPAN
TEL : +81-3-5632-9617
FAX : +81-3-5632-9618

ProteNova Co.Ltd. Takamatsu Lab.
2217-44 Hayashi-cho, Takamatsu
Kagawa 761-0301 Japan
TEL +81-87-897-2073 FAX +81-87-816-2073
URL <http://protenova.com>

Ab-Rapid PuRe Specifications

- Gel volume: 0.5 mL
- Gel matrix: 4% cross-linked agarose (Sephacrose 4 Fast Flow)
- Particle size: 45-165 μm
- Ligand: Alkali-resistant Protein A-derivatives (Protein A-R28) (*E. coli*)
- Binding Capacity: >65 mg human IgG /mL gel
- Storage: 20% Ethanol at 4-8 °C
- Accessories: Luar lock adaptor
2.5 mL syringe

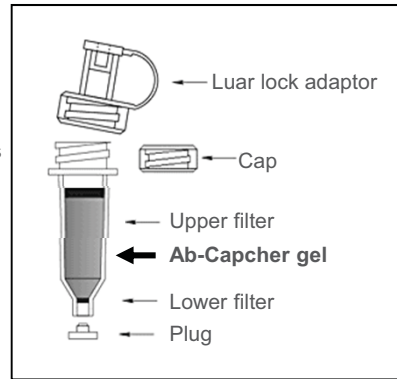

Materials

- 2.5 mL syringe
- Microcentrifuge tube
- Buffers
 - Binding Buffer: PBS
 - Elution Buffer: 0.1 M Glycine-HCl, pH 2.8
 - Neutralization Buffer: 1 M Tris

*** If air appeared in the space between gel and column**
Before use, pass through 10 mL of Binding Buffer into the column by using 10 mL syringe (flow-rate 5mL/min). It is important to apply pressure to the column. Repeat this procedure until air disappeared from the column.

- * Buffer Kit (PN-011) is also available from ProteNova.
Buffer kit contains Binding Buffer, Elution Buffer and Neutralization Buffer.

Sample preparation (example)

- ◆ Ascites : 3 x dilution with Binding Buffer.
- ◆ Serum : Ppt. with 50%-saturated $(\text{NH}_4)_2\text{SO}_4$ or 5 x dilution with Binding Buffer
- ◆ Cultured medium : Adjust pH to neutral.

Recommended pre-treatments of sample before applying to column.

- Centrifugation ; 10,000 $\times g$, 10 min
- Filtration ; 0.45 μm filter
(Please use low-protein-adsorption types)

- * If there are insolubles in the sample, make sure to do pre-treatments.

Preparation for 50% ammonium sulfate precipitation


1. Prepare saturated ammonium sulfate.
Add equal volume of saturated ammonium sulfate gradually to serum and mix.
2. Stand on ice for more than 1hr.
3. After centrifugation at 4°C, remove the supernatant.
Wash precipitate with 50%-saturated ammonium sulfate.
4. Resolve the precipitate with small volume of Binding Buffer. The precipitate contains antibody.
5. Exchange to Binding buffer with dialysis or desalting column.

Protocol for Antibody Purification

Preparation

Add Neutralization Buffer into a microcentrifuge tube.
(1/30 volume of eluate; 30-35 μL to 1 mL of eluate)

Remove a cap on the top of column and fit a luar lock adaptor.

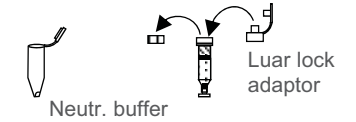


Step 1. Equilibration of Column

Fill a syringe with 2.5 mL of Binding Buffer and connect to the top of column.

After removal of a seal and a plug from the bottom of column, pass through 2.5 mL of Binding Buffer at a flow rate of 2.5 mL/min.


Then, remove the syringe.

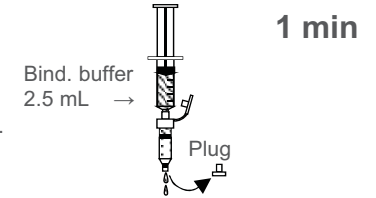

Step 2. Sample Apply to Column

Apply the sample solution to column using the syringe at a flow rate of 2 mL/min.

Then, remove the syringe.

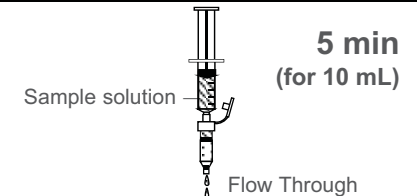


Step 3. Washing of Column

Wash the column with 2.5 mL of Binding Buffer with the syringe at a flow rate of 2.5 mL/min.

* If serum was directly applied to the column, washing of more than 5 mL is recommended.


Then, remove the syringe.

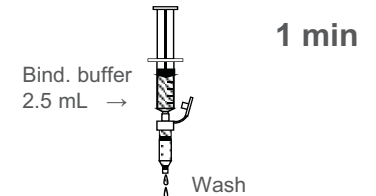

Step 4. Elution of IgG

Elute with 2 mL of Elution Buffer using the syringe at a flow rate of 2 mL/min.

For this, discard first 0.3-0.5 mL of eluate and collect the following 1.0 – 1.5 mL of eluate as IgG fraction into a microcentrifuge tube, in which Neutralization Buffer (1/30 volume of eluate) is pre-added, and mix.

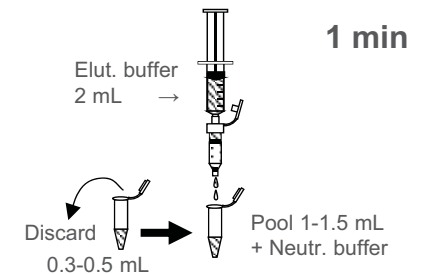

Time: within 10 min

* Storage and reuse of column

- Ab-Rapid PuRe column is alkali-washable.
- When the column is reused, wash the column with 2.5 mL of 0.1N NaOH by syringe after elution of IgG. Using immediately after washing, equilibrate with 2.5 mL of Binding Buffer twice. Then, apply the sample.
- For storage of column, add 2.5 mL of 20% EtOH, tightly close a cap and a plug, and store at 4-8°C.